Correction to: Simple motion correction strategy reduces respiratory-induced motion artifacts for k-t accelerated and compressed-sensing cardiovascular magnetic resonance perfusion imaging

Zhou, Ruixi ; Huang, Wei ; Yang, Yang ; Chen, Xiao ; Weller, Daniel S ; Kramer, Christopher M ; Kozerke, Sebastian ; Salerno, Michael

DOI: https://doi.org/10.1186/s12968-018-0439-x

Originally published at:
Zhou, Ruixi; Huang, Wei; Yang, Yang; Chen, Xiao; Weller, Daniel S; Kramer, Christopher M; Kozerke, Sebastian; Salerno, Michael (2018). Correction to: Simple motion correction strategy reduces respiratory-induced motion artifacts for k-t accelerated and compressed-sensing cardiovascular magnetic resonance perfusion imaging. Journal of Cardiovascular Magnetic Resonance, 20(1):23.
DOI: https://doi.org/10.1186/s12968-018-0439-x

Journal of Cardiovascular Magnetic Resonance

CORRECTION

Open Access

Correction to: Simple motion correction strategy reduces respiratory-induced motion artifacts for k-t accelerated and compressed-sensing cardiovascular magnetic resonance perfusion imaging

Ruixi Zhou[1,2†], Wei Huang[1†], Yang Yang[1,2], Xiao Chen[3], Daniel S. Weller[4], Christopher M. Kramer[1,5], Sebastian Kozerke[6] and Michael Salerno[1,2,5*]

Correction

Figure 1 of this original publication [1] contained a minor error as one of the lines in the "Reconstruction pipline" was not visible. The updated Fig. 1 is published in this correction article.

Author details
[1]Department of Medicine, University of Virginia Health System, Charlottesville, VA, USA. [2]Department of Biomedical Engineering, University of Virginia Health System, Charlottesville, VA, USA. [3]Medical Imaging Technologies, Siemens Healthineers, Princeton, NJ, USA. [4]Department of Electrical and Computer Engineering, University of Virginia, Charlottesville, VA, USA. [5]Department of Radiology and Medical Imaging, University of Virginia Health System, Charlottesville, VA, USA. [6]Department of Information Technology and Electrical Engineering, Institute for Biomedical Engineering, University and ETH Zurich, Zurich, Switzerland.

Received: 7 February 2018 Accepted: 19 February 2018
Published online: 26 March 2018

Reference

1. Zhou R, Huang W, Yang Y, et al. Simple motion correction strategy reduces respiratory-induced motion artifacts for k-t accelerated and compressed-sensing cardiovascular magnetic resonance perfusion imaging. J Cardiovasc Magn Reson. 2018;20:6. https://doi.org/10.1186/s12968-018-0427-1.

* Correspondence: ms5pc@virginia.edu
†Equal contributors
[1]Department of Medicine, University of Virginia Health System, Charlottesville, VA, USA
[2]Department of Biomedical Engineering, University of Virginia Health System, Charlottesville, VA, USA

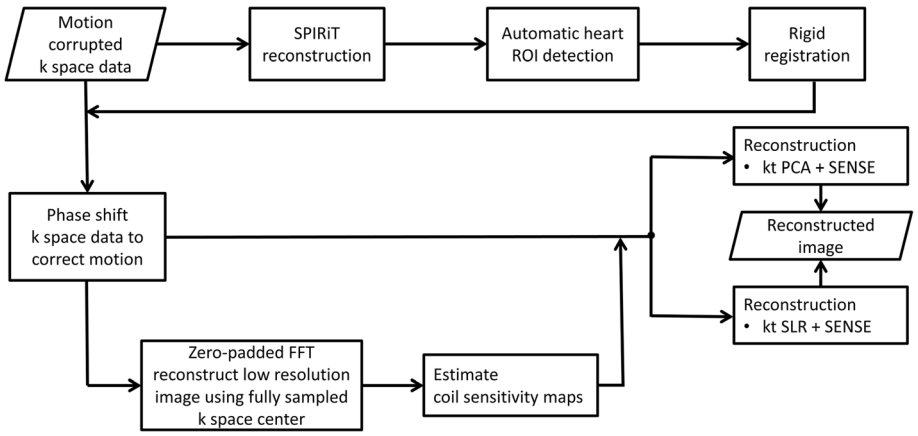

Fig. 1 Corrected Reconstruction pipeline